

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 7346 (1987): Raspatories, Rib, Semb's Pattern [MHD 6: Thoracic and Cardiovascular Surgery Instruments]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”

BLANK PAGE



Indian Standard

SPECIFICATION FOR RASPATORIES, RIB, SEMB'S PATTERN

(First Revision)

1. Scope — Specifies requirements and tests for Semb's pattern rib raspatories used in thoracic surgery.

2. Material — Stainless steel conforming to Designation 20Cr13 or 30Cr13 of IS : 6603-1972 'Specification for stainless steel bars and flats'.

3. Shapes and Dimensions — As shown in Fig. 1 and 2.

3.1 Tolerances on various dimensions shall be in accordance with the following:

- ± 0.05 mm on dimensions up to 2.0 mm,
- ± 0.1 mm on dimensions above 2.0 mm and up to 5.0 mm,
- ± 0.2 mm on dimensions above 5.0 mm and up to 20.0 mm,
- ± 0.5 mm on dimensions above 20.0 mm and up to 50.0 mm,
- ± 1.0 mm on dimensions above 50.0 mm and up to 100.0 mm, and
- ± 2.0 mm on dimensions above 100.0 mm.

4. Heat Treatment — The instruments shall be uniformly hardened and tempered to a hardness of 350 to 490 HV, when tested in accordance with IS : 1501 (Part 1)-1984 'Method for Vickers hardness test for metallic materials : Part 1 HV 5 to HV 100 (second revision)'.

5. Workmanship — All edges and corners, except the scraping edge, shall be rounded. The scraping edge shall be semi-sharp.

6. Surface Condition

6.1 General — All surfaces shall be free from pores, crevices and grinding marks. The instruments shall be supplied free from residual scales, acid, grease, and grinding and polishing materials. Compliance with these requirements shall be checked by inspection using normal vision (corrected, if necessary).

6.2 Surface Finish — The surface finish shall be one of, or a combination of, the following:

- Mirror polished;
- Reflection-reducing, for example, satin finish, matt black finish; and
- An applied surface coating, for example, for insulation purposes.

Note — The satin finish should be effected by an appropriate procedure, such as grinding, brushing, electropolishing and, in addition, satin finishing (glass beading or satin brushing). The finish should be uniform and smooth and it should reduce glare.

Instruments of mirror finish should be adequately ground to remove all surface imperfections and polished to remove grinding marks, resulting in a mirror finish. The mirror finish should be effected by an appropriate procedure, such as polishing, brushing, electropolishing, and mirror buffing.


6.3 Passivation and Final Treatment — The instrument shall be treated by a suitable passivation process, for example, by electropolishing or by treatment with 10 percent (v/v) nitric acid solution for not less than 30 minutes at a temperature not less than 10°C and not exceeding 60°C. The instrument shall then be rinsed in water and dried in hot air.

7. Tests

7.1 View Under Magnification — The scraping edge of the raspatory shall be examined under a magnification of $\times 10$. The edge shall be well-defined and free from any defect.


7.2 Sharpness Test — The scraping edge of the raspatory shall be run on a well-seasoned teak wood surface along the grain or on unfinished side of hard leather. The raspatory shall scrape the surface and not dig into the wood or leather.

7.3 Corrosion Resistance Test — The instrument shall be tested in accordance with IS : 7531-1975 'Method for boiling and autoclaving test for corrosion resistance of stainless steel surgical instruments'. They shall show no sign of corrosion after the test.

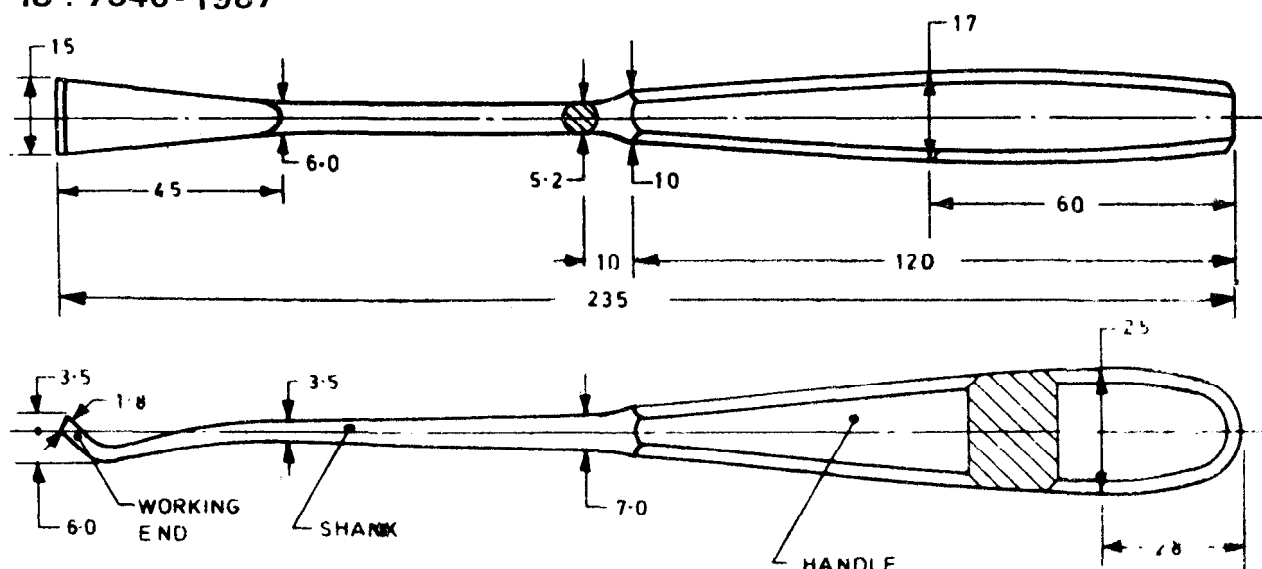

All dimensions in millimetres.

FIG. 1 RASPATORY, RIB, SEMB'S PATTERN, CHISEL EDGE

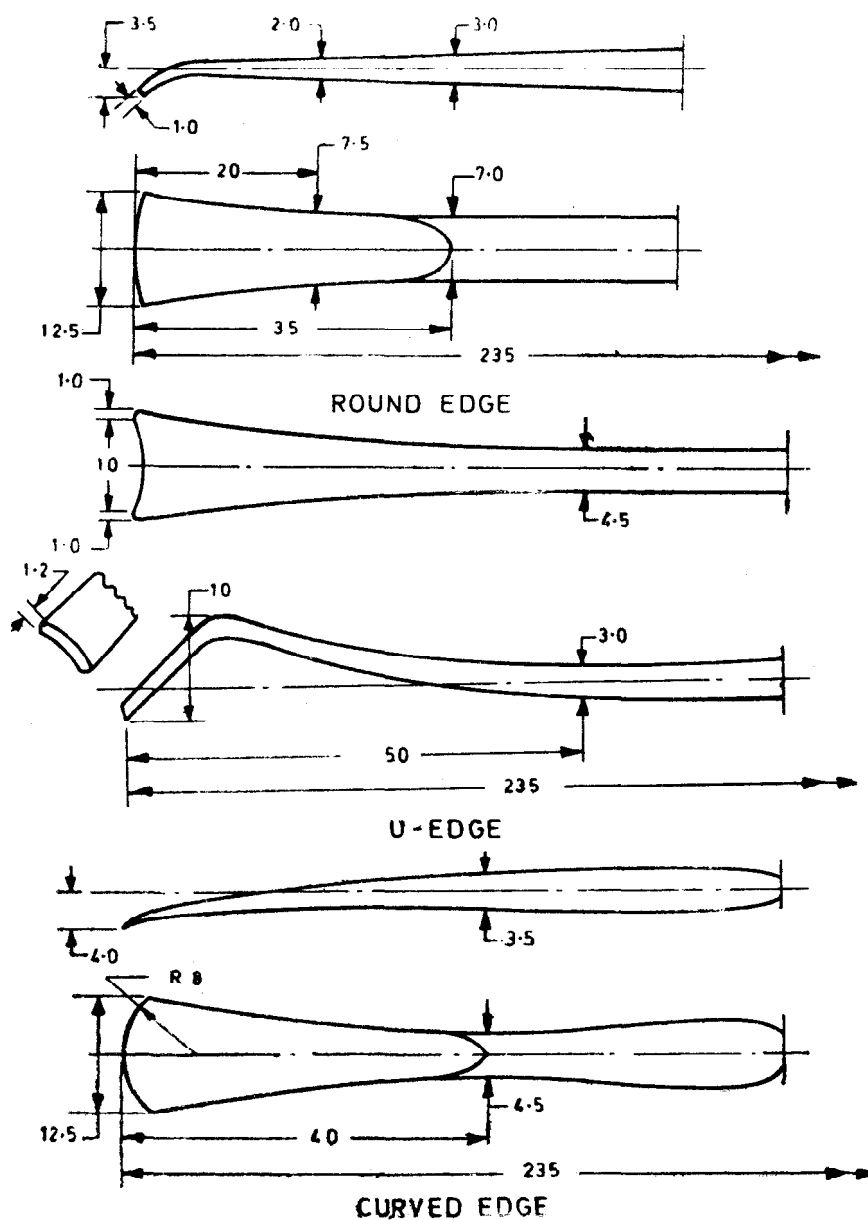

All dimensions in millimetres.

FIG. 2 RASPATORIES, RIB, SEMB'S PATTERN, VARIOUS EDGES

8. Marking and Packing

8.1 The instrument shall be legibly and indelibly marked with the manufacturer's name, initials or recognized trade-mark; the words 'Stainless Steel' or letters 'SS'; and the country of manufacture.

8.2 Each instrument shall be put in a polyethylene bag or wrapped in wax paper. The instruments shall then be packed in cartons in accordance with the current trade practice.

8.2.1 Alternatively, the instruments may be packed as agreed to between the purchaser and the supplier.

8.3 The packages shall be marked with the name of the instrument and the shape of its edge; manufacturer's name, initials or recognized trade-mark; the words 'Stainless Steel'; and the country of manufacture.

8.4 *Standard Marking* — Details available with the Bureau of Indian Standards.

9. Sampling — The scale of sampling and criteria for conformity of the instruments to the requirements of this specification shall be as agreed to between the purchaser and the supplier. A recommended sampling plan is given in Appendix A.

APPENDIX A

(Clause 9)

SAMPLING OF RASPATORIES, RIB, SEMB'S PATTERN

A-1. Lot — In any consignment, all the instruments with the same shape of the edge, produced from the identical material under similar conditions and having the same surface finish shall constitute a lot.

A-2. The number of instruments to be selected from each lot shall depend upon the size of the lot and shall be in accordance with col 1 and 2 of Table 1.

TABLE 1 SCALE OF SAMPLING

(Clauses A-2, A-3.1 and A-3.2)

Lot Size (1)	Sample Size (2)	Sub-Sample Size (3)
Up to 15	2	1
16 to 50	3	1
51 to 150	5	2
151 and above	8	3

A-2.1 These instruments shall be selected from the lot at random and in order to ensure randomness of selection, procedure given in IS : 4905-1968 'Methods for random sampling', may be followed.

A-3. Number of Tests and Criteria for Conformity

A-3.1 All the instruments selected according to col 1 and 2 of Table 1 shall be examined for shape and dimensions, workmanship, surface condition (visual) and view of the scraping edge under magnification. An instrument in the sample failing to meet any of these requirements shall be considered as defective. The lot shall be considered as conforming to these requirements if no defective is found in the sample.

A-3.2 The lot having been found satisfactory according to **A-3.1** shall be further tested for other requirements. For this purpose, a sub-sample of size given in col 3 of Table 1 shall be taken. These instruments in the sub-sample may be selected from those already examined according to **A-3.1**. Each instrument in the sub-sample shall be subjected to hardness, sharpness and corrosion resistance tests. The lot shall be declared as conforming to the requirements of the specification if none of the instruments in the sub-sample fails in any of these tests.

EXPLANATORY NOTE

This standard was first issued in 1974. In this revision, requirements for material have been altered, tolerances on various dimensions have been specified, a recommended sampling plan has been added and the clauses on surface condition have been modified besides incorporating certain other modifications.

AMENDMENT NO. 1 NOVEMBER 1990
TO
IS 7346:1987 SPECIFICATION FOR
RASPATORIES, RIB, SEMB'S PATTERN

(First Revision)

(Page 1, clause 2, line 1) Delete the words
'20Cr13 or'.

(MHD 6)

Reprography Unit, BIS, New Delhi, India